Because we care.

MIDMARK®

Installation / Operation

Model 4745-001 ECG Cart

KIT COMPONENTS

Part Number	Description	Qty
4745-001	ECG (Electrocardiograph) Cart	1
003-1098-00	Installation / Operation Instructions	1

REQUIRED TOOLS

None

INTRODUCTION

To provide a mobile support surface for an electrocardiograph device or other device of comparable size and weight.
The cart has a five caster base with three swivel and two locking casters.
Maximum top weight capacity is 40 lbs. (18.1 Kgs.) centered on top.
Maximum drawer weight capacity 10 lbs. (4.5 Kgs.)
There are no accessories.

CE REPRESENTATIVE

EEC countries should direct all questions, incidents, and complaints to Midmark authorized CE representative:

Promotal
22, Rue De St. Dines
53500 Ernie
France
Phone: 33-2-430-517-76
Fax: 33-2-430-569-10

INSTALLATION

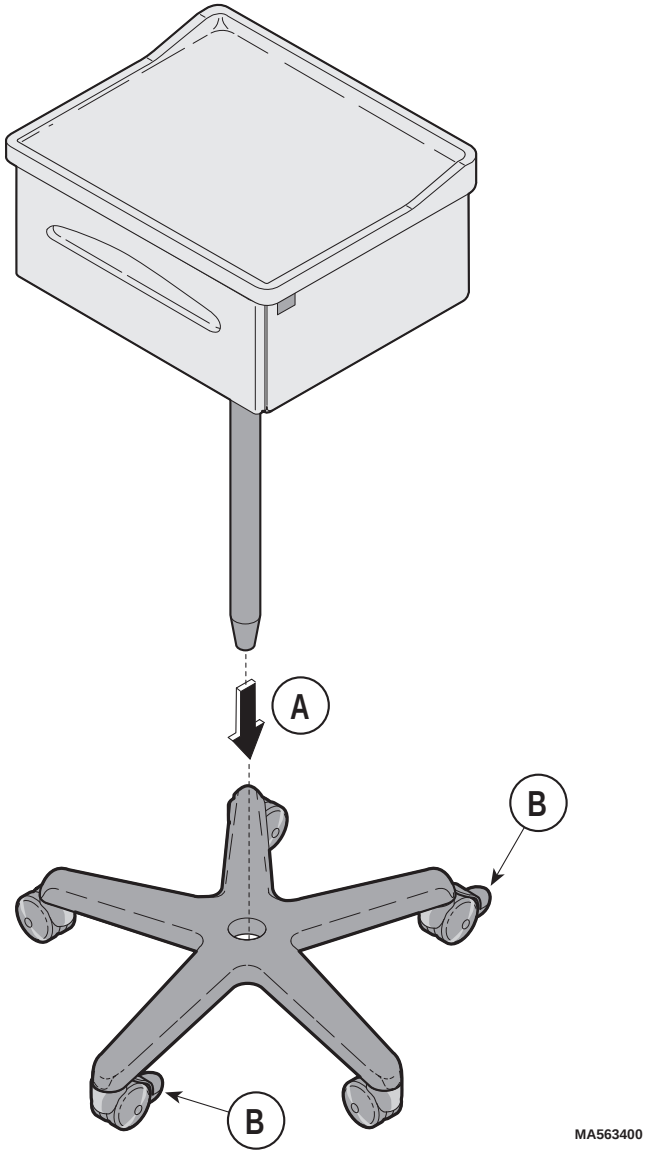

A. Insert pedestal into caster base, pressing firmly downward.

B. Release two locking casters and check operation.

© Midmark Corporation - 2000

PARTS

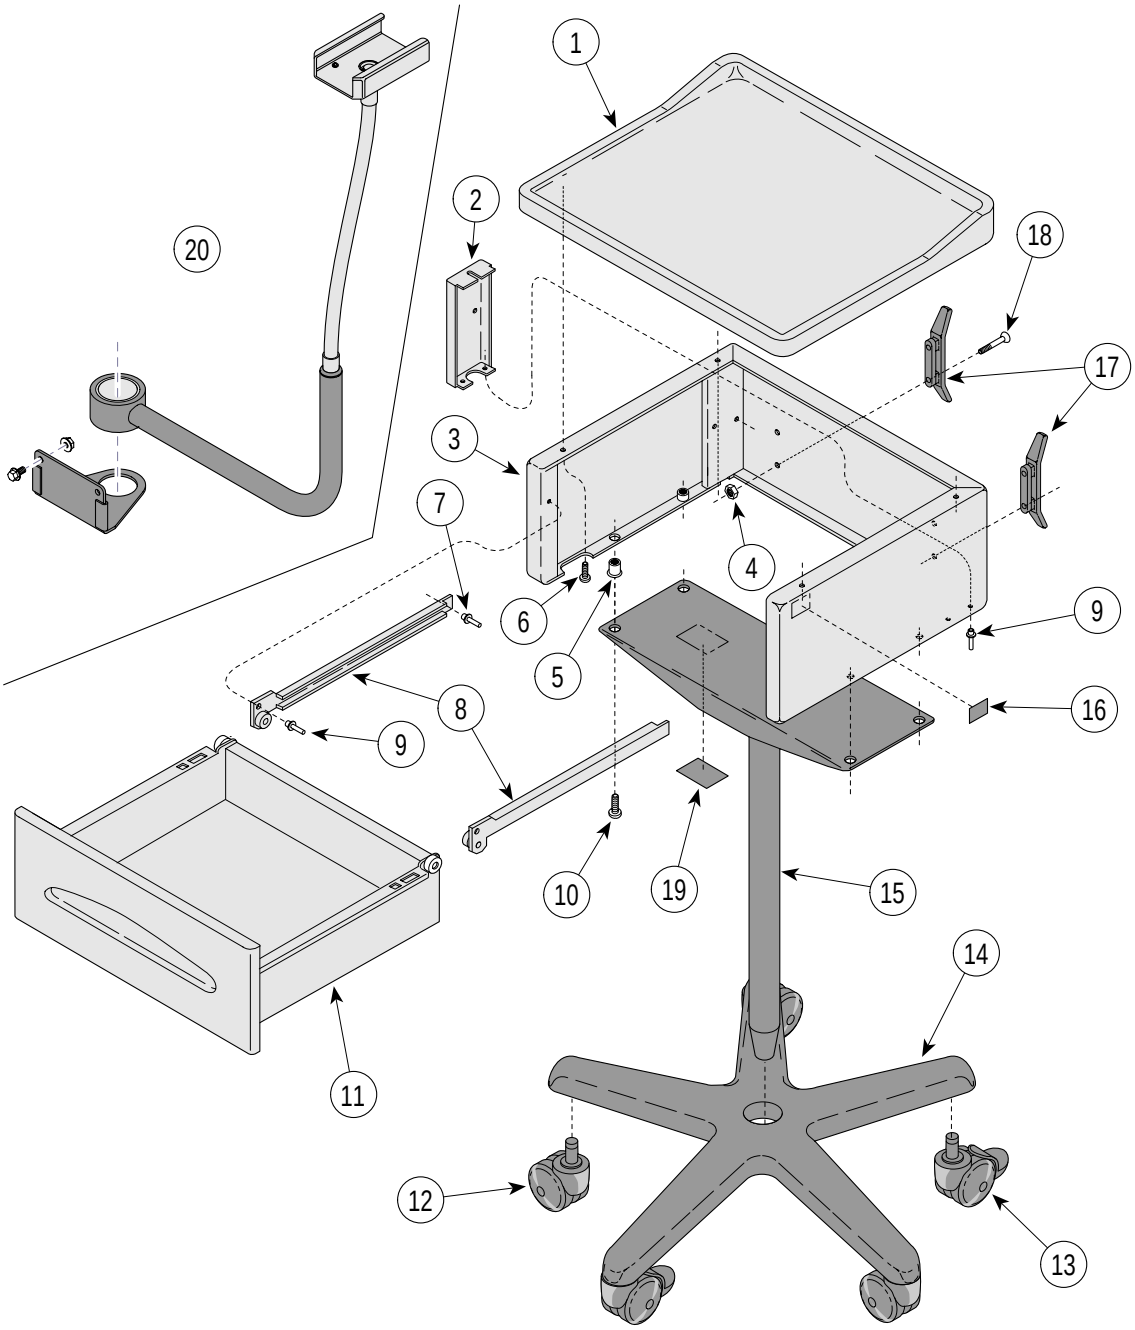

MA562401

Item	Part No.	Description	Qty.
	4745-001	ECG Cart (Includes Items 1 thru 19)	1
1	• 063-9939-00	• ECG Cart Top	1
2	• 050-4795-50	• Slide Support	2
3	• 050-4889-50	• Cart Drawer Cover	1
4	• 041-0008-02	• Nylock Nut	4
5	• 042-0045-06	• Nutsert	4
6	• 040-0010-48	• Particle Board Screw	4
7	• 042-0010-27	• Countersunk Head Pop Rivet	2
8	• 016-0813-04	• Drawer Slide / Runner Set	1
9	• 042-0010-04	• Pop Rivet	6
10	• 040-0250-88	• Screw	4

Item	Part No.	Description	Qty.
11	• 029-2534-00	• Drawer Assembly	1
12	• 016-0884-00	• Caster	3
13	• 016-0883-00	• Locking Caster	2
14	• 016-0681-00	• Base	1
15	• 030-1278-00	• Post Weldment	1
16	• 061-0759-02	• Midmark Label	1
17	• 016-0864-00	• Plastic Rope Clete	2
18	• 040-0008-100	• Screw	4
19	•	• Serial Number Label	1
20	9A283001	IQMark Flexible Rotating Mount Holder (Optional Accessory)	1

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

© Midmark Corporation - 2000